

Spis treści

Termometr TB63o; 0-120°C; opaskowy (T78835)	2
Termometr TB63T; 0-120°C; R40; G12 (7E697)	3
Termometr TB63T; 0-120°C; R50; G1 2 (T5540)	4
Termometr TB63T; 0-120°C; R60; G12 (02C42)	5
Termometr TB63T; 0-120°C; R100; G12 (T2829)	6
Termometr TB100R; 0-120 C; R50; G12 (T70986)	7
Termometr TB100T; 0-120C; R50; G12 (T97067)	8
Termometr TB100T; 0-120°C; R63; G12 (653CB)	9
Termometr TB100T; 0-120°C; R80; G12 (8A037)	10
Termometr TB100T; 0-120°C; R160; G1 2 (D26D0)	11
Termometr TB100T; 0-150°C; R50; G1 2 (35770)	12
Termometr TB100T; 0-150C; R63; G1 2 (19169-33F51)	13
Termometr TB100T; 0-150°C; R100; G1 2 (74681)	14
Termometr TB100T; 0-150°C; R160; G12 (T641U0252)	15



Termometr TB63o; 0-120'C; opaskowy; **T78835**



Termometr TB63T; 0-120°C; R40; G1/2"; **TRMMT-63090-7E697**



Termometr TB63T; 0-120°C; R50; G1/2"; **T5540**



Termometr TB63T; 0-120°C; R60; G1/2"; **TRMMT-63064-02C42**



Termometr TB63T; 0-120°C; R100; G1/2"; **T2829**



Termometr TB100R;
0-120°C; R50; G1/2"
T70986



Termometr TB100T; 0-120°C;
R50; G1/2"; **T97067**



Termometr TB100T; 0-120°C; R63; G1/2"; **100ED-653CB**




Termometr TB100T; 0-120'C; R80; G1/2"; **8A037**



Termometr TB100T; 0-120°C; R160; G1/2"; **231FB-D26D0**



Termometr TB100T; 0-150°C; R50; G1/2"; **35770**

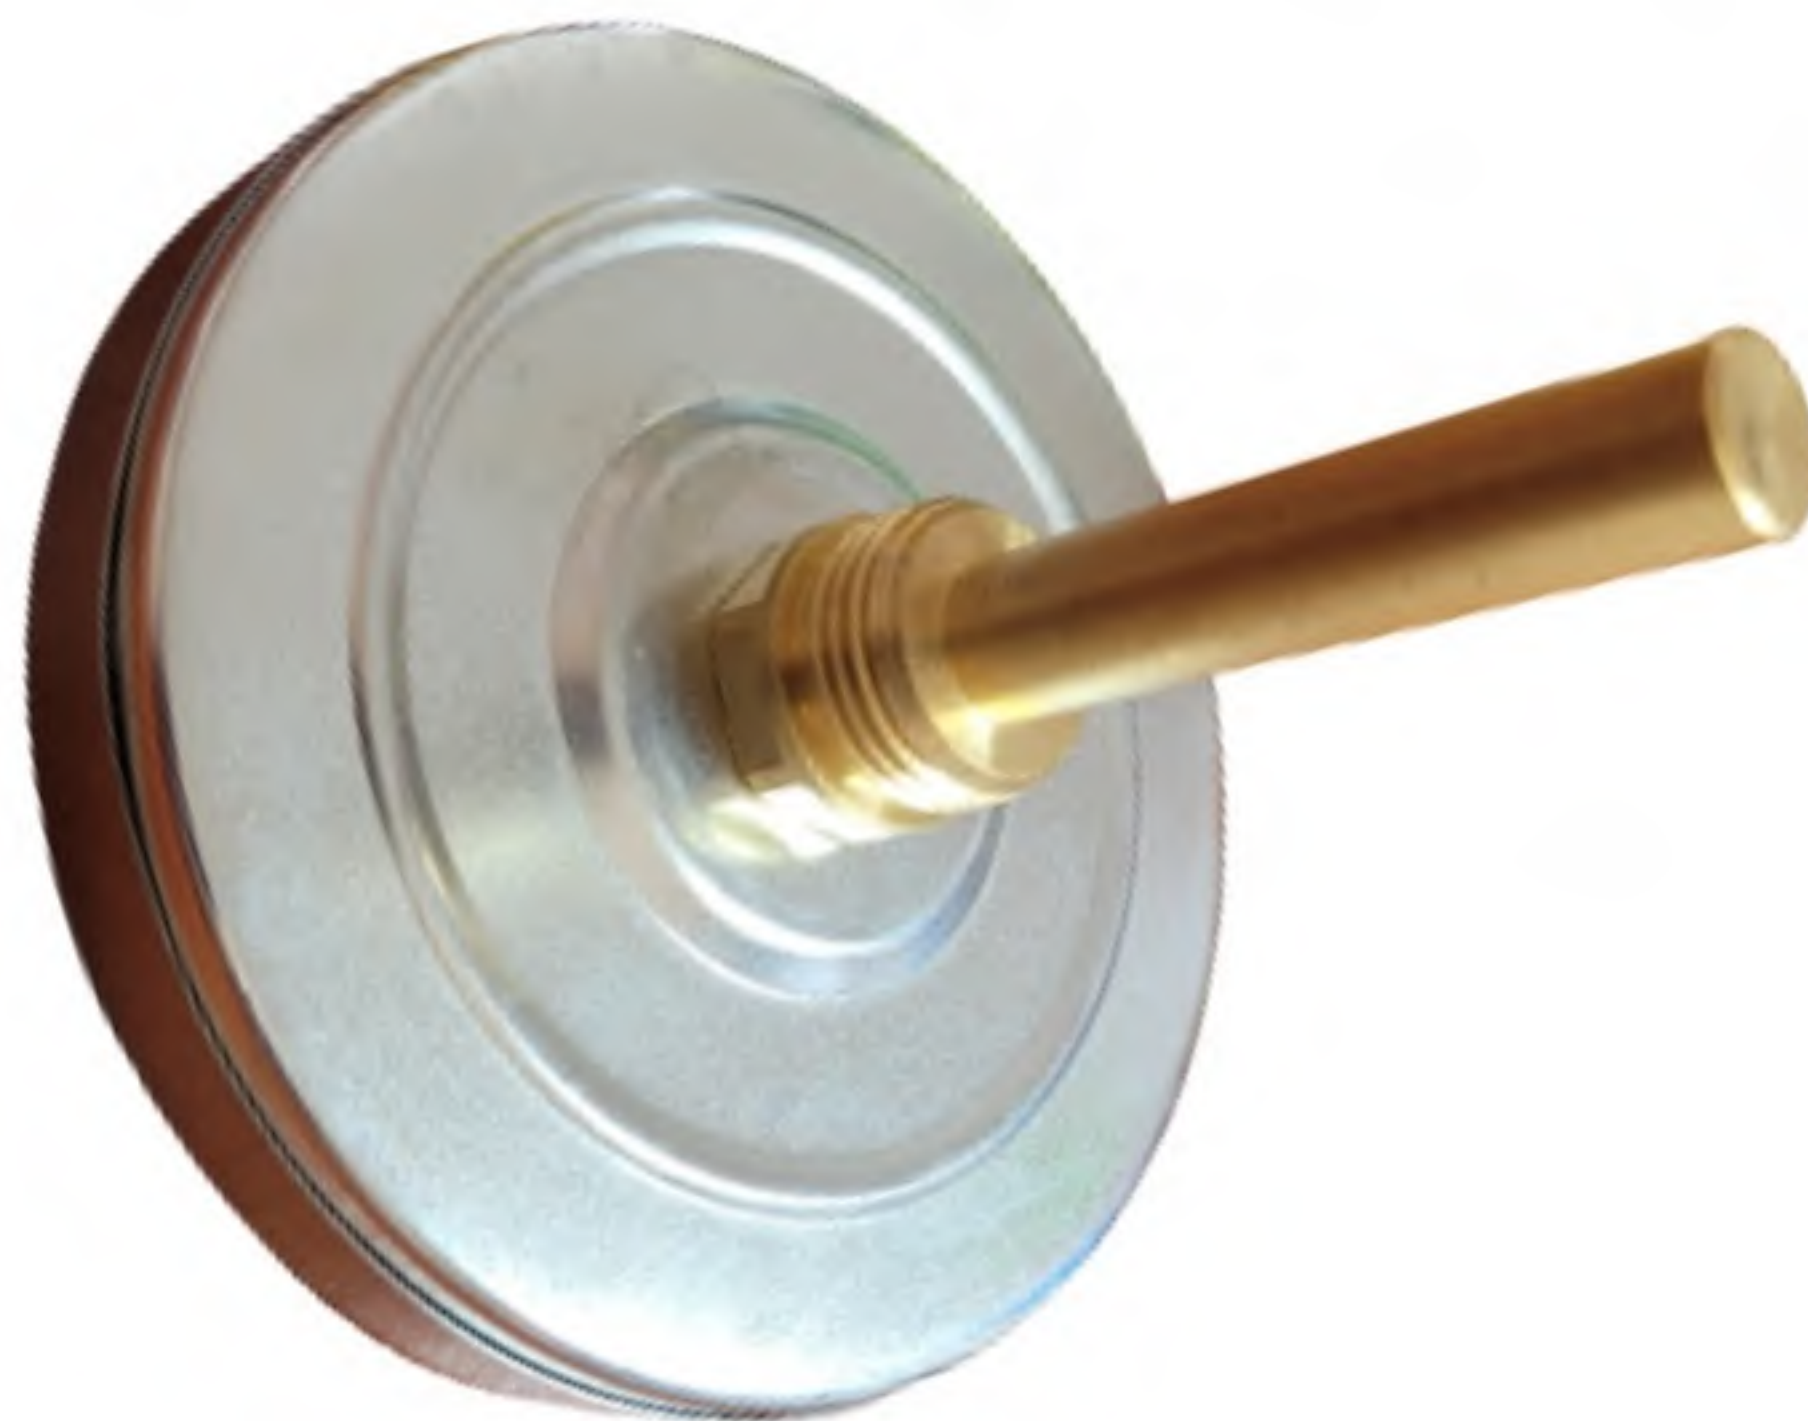

Termometr TB100T; 0-150°C;
R63; G1/2"; **19169-33F51**



Termometr TB100T; 0-150°C;
R100; G1/2"
74681



Termometr TB100T; 0-150°C; R160; G1/2"; **641U0252**